



Tube Watch for SPECT/CT StarGuide™

Reduce disruptions. Enhance care.



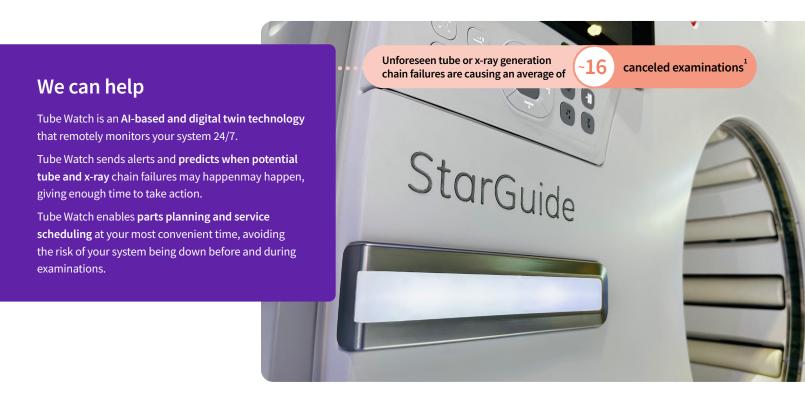

Innovative technologies that help predict and prevent failures on StarGuide Platform

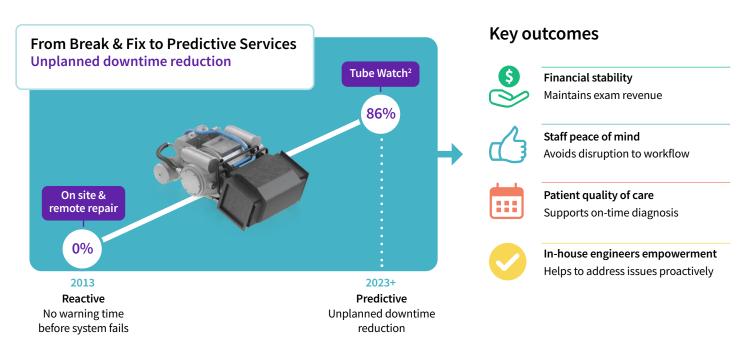

- Number of cancelled examination is based on the average utilization of a SPECT/CT scanner across USCAN
 and EMEA in the last 12 rolling months (source is iCenter) compared to the average downtime which is calculated
 based on 110 X-ray tube failures in EMEA and USCAN in 2023 and 2024 and calculated on a 24x7.
- 2. Percentage noted is based on various assumptions, including but not limited to the use of Tube Watch consistent with the Tube Watch terms and conditions, timely receipt of the tube-health notice, parts and labor availability, immediate access to customer's equipment, and may not be typical of every customer's experience. Recommended replacement lead time of the X-ray Tube might increase in case of specific options installed on the system.

Not all products or features are available in all markets. Contact a GE HealthCare Representative for more information. Please visit http://www.gehealthcare.com. Data subject to change.

© 2024 GE HealthCare.

iCenter, OnWatch, StarGuide, and Tube Watch are trademarks of GE HealthCare. GE is a trademark of General Electric Company used under trademark license.

JB30408XX | October 2024

